


SECTION AROUND PERIMETER

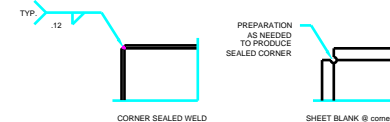

SIDING PREPARATION TYPICAL DETAIL

SCALE= 1:2

- NOTES:**
1. LEAD PANELS SHALL BE CONSTRUCTED FROM SINGLE UNPERFORATED SHEET, FREE OF CRACK, INCLUSIONS, FISSURES, VOIDS AND ALL OTHER DETRIMENTAL DEFECTS. MATERIAL SHALL BE LEAD GRADE "C" TO COMPLY WITH FEDERAL SPECIFICATION 48021.2. MATERIAL SHALL BE ALL APPLICABLE FEDERAL, STATE AND LOCAL RADIATION GUIDE LINES: NBS HANDBOOK 111 AND 114, ANSI N43.2 AND DOE ORDER 5400.11
 2. FINISH - PAINT EXTERIOR SURFACES, EXCEPT AS NOTED, WITH PRATT & LAMBERT #2127 (SNO-FLAKE WHITE, SEMI-GLOSS, EPOXY BASE) OR EQUIVALENT. SURFACE PREPARATION PER A.N.L. SPECIFICATION #4105-000-024.
 3. DIMENSIONS IN BRACKETS [] ARE MILLIMETERS AND ARE FOR REFERENCE ONLY.
 4. SOME HIDDEN LINES MAY BE OMITTED FOR CLARITY.

DETAIL 1
LOW CARBON STEEL

[illegible]